



# The Brazilian Journal of INFECTIOUS DISEASES

[www.elsevier.com/locate/bjid](http://www.elsevier.com/locate/bjid)



## Original article

# Detection of the *mecA* gene and identification of *Staphylococcus* directly from blood culture bottles by multiplex polymerase chain reaction



Taisa Trevizani Rocchetti<sup>a,b,\*</sup>, Katheryne Benini Martins<sup>a</sup>,  
Patricia Yoshida Faccioli Martins<sup>a</sup>, Rogério Antonio de Oliveira<sup>c</sup>,  
Alessandro Lia Mondelli<sup>d</sup>, Carlos Magno Castelo Branco Fortaleza<sup>b</sup>,  
Maria de Lourdes Ribeiro de Souza da Cunha<sup>a</sup>

<sup>a</sup> UNESP - Univ Estadual Paulista, Instituto de Biociências de Botucatu, Departamento de Microbiologia e Imunologia, Botucatu, SP, Brazil

<sup>b</sup> UNESP - Univ Estadual Paulista, Faculdade de Medicina de Botucatu, Hospital Universitário, Departamento de Doenças Tropicais, Botucatu, SP, Brazil

<sup>c</sup> UNESP - Univ Estadual Paulista, Instituto de Biociências de Botucatu, Departamento de Biociência, Botucatu, SP, Brazil

<sup>d</sup> UNESP - Univ Estadual Paulista, Faculdade de Medicina de Botucatu, Hospital Universitário, Departamento de Medicina Interna, Botucatu, SP, Brazil

## ARTICLE INFO

### Article history:

Received 3 November 2017

Accepted 18 February 2018

Available online 13 March 2018

### Keywords:

*Staphylococcus* spp.

*Staphylococcus aureus*

MRSA

*mecA* gene

Blood cultures

Multiplex PCR

## ABSTRACT

**Introduction:** *Staphylococcus* spp. – both *S. aureus*, including methicillin-resistant strains (MRSA) and coagulase negative staphylococci (CoNS) – are relevant agents of healthcare-associated infections. Therefore, the rapid recognition of MRSA and methicillin-resistant CoNS from blood stream infections is critically important for patient management. It is worth noting that inappropriate empiric therapy has been associated with higher in-hospital mortality.

**Material and methods:** In this study we evaluated a multiplex polymerase chain reaction (multiplex PCR) standardized to detect *Staphylococcus* spp., *S. aureus*, and *mecA* gene-encoded oxacillin resistance directly from blood culture bottles. A total of 371 blood cultures with Gram-positive microorganisms confirmed by Gram-stain were analyzed. Results from multiplex PCR were compared to phenotypic characterization of isolates.

**Results:** *Staphylococcus aureus* was detected in 85 (23.0%) blood cultures and CoNS in 286 (77.0%). There was 100% agreement between phenotypic and multiplex PCR identification. Forty-three (50.6%) of the 85 *S. aureus* carried the *mecA* gene and among the 286 CoNS, 225 (78.7%) were positive for the *mecA* gene.

\* Corresponding author.

E-mail address: [taisa\\_texrocchetti@hotmail.com](mailto:taisa_texrocchetti@hotmail.com) (T.T. Rocchetti).

<https://doi.org/10.1016/j.bjid.2018.02.006>

1413-8670/© 2018 Sociedade Brasileira de Infectologia. Published by Elsevier Editora Ltda. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

**Conclusions:** The multiplex PCR assay developed here was found to be sensitive, specific, rapid, and showed good agreement with the phenotypic results besides being less expensive. This PCR method could be used in clinical laboratories for rapid identification and initiation of specific and effective treatment, reducing patient mortality and morbidity. Furthermore, this method may reduce misuse of antimicrobial classes that are more expensive and toxic, thus contributing to the selection of antibiotic-resistant *Staphylococcus* spp.

© 2018 Sociedade Brasileira de Infectologia. Published by Elsevier Editora Ltda. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

## Introduction

Sepsis is the systemic response to infection and is the result of the complex interaction between the host's immune system and the infecting microorganism.<sup>1</sup> Many bacteria are isolated from bloodstream infections, including Gram-positive and Gram-negative bacteria. According to the US Centers for Disease Control and Prevention (CDC),<sup>2</sup> a clear change in the nature of the infectious microorganisms has occurred over the past decade, when Gram-positive cocci have exceeded Gram-negative bacilli as the main etiological agents of sepsis and *Staphylococcus* spp. have become the most prevalent agents.

The genus *Staphylococcus* comprises 52 species<sup>3</sup>; of these, 17 can be isolated from human biological samples. The genus can be divided into two main groups: coagulase-positive staphylococci, whose main member is *S. aureus*, and coagulase-negative staphylococci (CoNS). *Staphylococcus aureus* possesses a wide variety of virulence factors, including peptidoglycan, teichoic acid, enzymes and toxins, adhesion molecules, and four types of cytotoxins.<sup>4</sup> They can cause different types of infection, many of them acquired in the hospital environment. About 20% to 30% of the human population is colonized with this bacterium and the nasal mucosa is the main ecological niche.<sup>5</sup>

A relevant factor that complicates treatment of staphylococcal infections is the high resistance rate to  $\beta$ -lactam antibiotics observed among *Staphylococcus* spp., which requires large-scale use of expensive or toxic antibiotics. *Staphylococcus* spp. resistance to  $\beta$ -lactam antibiotics is mainly due to two different mechanisms which, however, can interact. The first mechanism consists of the production of  $\beta$ -lactamase, an enzyme that hydrolyzes the antibiotic. The second mechanism is related to a change in the site of action of  $\beta$ -lactams by producing a new penicillin-binding protein, PBP2a, which has low affinity for antibiotics and is absent in susceptible staphylococci.<sup>6</sup> PBP2a is encoded by the *mecA* gene. This gene is located on a mobile genetic element called SCC*mec* (staphylococcal cassette chromosome *mec*), which is widely distributed among staphylococci.<sup>7</sup> PBP2a acts as a transpeptidase that resumes cell wall synthesis functions when other PBPs are inhibited, thus ensuring the integrity of the bacterial cell in the presence of  $\beta$ -lactams.<sup>8</sup>

In view of the above considerations, rapid detection of bacteremia and the subsequent rapid identification of the bacteria involved and their susceptibility to antibiotics are of great

diagnostic and prognostic importance. Multiplex polymerase chain reaction (PCR) allows to amplify genes of multiple pathogens and more than one specific DNA sequence of each pathogen using multiple sets of primers in a single reaction. This technique permits rapid detection and is effective in identifying pathogenic microorganisms in clinical samples, especially those that require urgent initiation of treatment.

The aim of the present study was to evaluate the efficacy, accuracy and sensitivity of multiplex PCR in detecting *Staphylococcus* spp., *S. aureus*, and *mecA* gene-encoded oxacillin resistance directly from blood culture bottles.

## Material and methods

### Isolates

A total of 371 *Staphylococcus* spp. isolated from positive blood cultures between May 2011 and May 2012 were provided by the Laboratory of Microbiology at the Teaching Hospital of Botucatu Medical School, UNESP - Univ Estadual Paulista (City of Botucatu, São Paulo State, Brazil).

### Sample collection

The isolates included in the study were obtained on the day following growth detection in a Bactec 9120 system and after confirmation of containing probable *Staphylococcus* spp. by Gram staining (Gram-positive cocci) and positive catalase tests.

The blood culture bottles were disinfected with 70% alcohol and 3 mL of blood was collected with a 5 mL syringe and 70  $\times$  25-mm needle into two microtubes (1.5 mL per microtube). One microtube was used for seeding onto blood agar for phenotypic identification and the other microtube was used for extraction of bacterial DNA for multiplex PCR.

### Phenotypic identification of *S. aureus* and coagulase-negative staphylococci

Phenotypic identification was performed at the Laboratory of Bacteriology, Department of Microbiology and Immunology, Botucatu Biosciences Institute, UNESP. The samples were seeded into blood agar and incubated for 24 h at 37 °C. After isolation from blood agar, the bacteria were submitted to Gram staining for confirmation of morphological staining

characteristics, catalase test for characterization of the genus *Staphylococcus*, and coagulase test for differentiation between *S. aureus* and CoNS.

#### DNA extraction directly from blood culture

Before DNA extraction, the samples were treated to remove interfering elements in the blood culture. The sample was centrifuged at  $850 \times g$  for 2 min.<sup>9</sup> The supernatant was transferred to another microtube and again centrifuged at  $11,000 \times g$  for 1 min. The supernatant was carefully discarded, leaving only the pellet. Five hundred microliters of lysozyme buffer (1 M EDTA, 0.1 M NaCl, 10 mM Tris, pH 8.0, and 5% Triton X-100) was then added to the pellet and the mixture homogenized in a vortex. Next, 800  $\mu$ L benzyl alcohol (Sigma) was added, the mixture homogenized in a vortex, and the microtube centrifuged at  $7000 \times g$  for 5 min.<sup>10</sup> Two phases formed in the microtube, the lower phase contained the alcohol with interfering substances (inhibitors) and the upper phase the bacteria.

For DNA extraction, 320  $\mu$ L of the liquid was removed from the upper phase and transferred to another microtube and 10  $\mu$ L lysozyme was added (10 mg lysozyme in 1 mL 10 mM Tris-HCl). The microtube was homogenized in a vortex and incubated at room temperature for 15 min, homogenizing the microtube at five-minute intervals. After this period, 10  $\mu$ L proteinase K was added and the mixture was incubated for 15 min at 56 °C, homogenizing the microtube at five-minute intervals in a vortex. The liquid (330  $\mu$ L) was transferred to a silica column provided by the illustra extraction kit (GE Healthcare). This column was placed inside a tube and centrifuged at  $11,000 \times g$  for 1 min. Lysis solution (500  $\mu$ L) was added and the column centrifuged at  $11,000 \times g$  for 1 min. Next, 500  $\mu$ L washing solution was added and the column was again centrifuged at  $11,000 \times g$  for 3 min. The tube was discarded and the column was transferred to a microtube. Elution solution (200  $\mu$ L) pre-warmed to 70 °C in water bath was then added to the column. After incubation at room temperature for 1 min, the microtube was centrifuged at  $11,000 \times g$  for 1 min and the DNA obtained was stored in a freezer at -20 °C.

#### Antimicrobial susceptibility testing

The isolates were submitted to *in vitro* susceptibility testing by the disk diffusion method on Mueller-Hinton agar plates at the Laboratory of Microbiology, Department of Internal Medicine, University Hospital, Botucatu Medical School, UNESP, according to the Clinical and Laboratory Standards Institute criteria.<sup>11</sup>

#### Standardization of multiplex PCR for the detection of *Staphylococcus spp.*, *S. aureus*, and *mecA* gene

First, PCR was standardized using a range of annealing temperatures to establish the adequate annealing temperature for all primers (Table 1). Amplification was performed in an Eppendorf thermocycler. The amplification conditions were: 92 °C for 3 min, followed by 30 cycles of DNA denaturation at 92 °C for 1 min, annealing at 56 °C for 1 min, and extension at 72 °C for 3 min. The final reaction volume was 35  $\mu$ L containing

**Table 1 – Primers used for the detection of *Staphylococcus spp.*, *S. aureus* and the *mecA* gene by multiplex PCR.**

Gene	Primer	Amplicon(bp)
<i>S. aureus</i> <sup>24</sup>	SAU327 – GGA CGA CAT TAG ACG AAT CA SAU1645 – CGG GCA CCT ATT TTC TAT CT	1250
16S rRNA <sup>25</sup>	16S <sub>1</sub> – 5' CCTATAA- GACTGGGATAAAGTTTCGGG 3' 16S <sub>2</sub> – 3' CTTTGAGTTTCAAC- CTTGCGGTTCG 5'	791
<i>Coa</i> <sup>26</sup>	COA <sub>1</sub> – 5' GTA GAT TGG GCA ATT ACATTT TGG AGG 3' COA <sub>2</sub> – 5' CGC ATCAGC TTT GTT ATC CCA TGT A 3'	117
<i>mecA</i> <sup>27</sup>	MRS <sub>1</sub> – 5' AAAATC- GATGGTAAAGGTTGGC 3' MRS <sub>2</sub> – 3' AGTTCT- GCAGTACCGGATTTCG 5'	533

10.2  $\mu$ L autoclaved Milli-Q water, 3.5  $\mu$ L deoxyribonucleotide triphosphates (dNTP) (Life Technologies), 0.8  $\mu$ L Taq DNA polymerase (Biotools), 2.5  $\mu$ L MgCl<sub>2</sub>-free buffer (Biotools), 2.5  $\mu$ L MgCl<sub>2</sub> (Biotools), 0.14  $\mu$ M of each 16S primer, 0.86  $\mu$ M of each MRS primer, 0.35  $\mu$ M of each SAU primer, 0.57  $\mu$ M of each COA primer, and 3.5  $\mu$ L of bacterial DNA. The amplification products were analyzed by electrophoresis on 3% agarose gel at 70 V. The following controls were included in all amplification reactions: ATCC 33591 (*mecA*-positive *S. aureus*), ATCC 25923 (*mecA*-negative *S. aureus*), ATCC 12228 (*mecA*-negative *S. epidermidis*), and negative control (water).

#### Sensitivity test

The sensitivity of multiplex PCR was evaluated by amplifying serial dilutions of *S. aureus* and CoNS control strains, starting with a dilution of 10<sup>-1</sup> (corresponding to 10<sup>7</sup> CFU/mL) until 10<sup>-7</sup> (10 CFU/mL) based on a 0.5 McFarland standard (1.5  $\times$  10<sup>8</sup> CFU/mL).

#### Specificity test

The specificity of multiplex PCR was evaluated by PCR using strains of other microbial species isolated directly from a culture and from positive blood culture bottles containing other bacterial species. The following species were analyzed: *Enterococcus faecalis*, *Enterococcus faecium*, *Streptococcus viridans*, *Streptococcus pneumoniae*, *Candida spp.*, Gram-positive bacilli, *Pseudomonas aeruginosa*, *Escherichia coli*, *Klebsiella pneumoniae*, *Acinetobacter baumannii*, *Enterobacter cloacae*, *Enterobacter aerogenes*, *Salmonella spp.*, *Morganella morganii*, and *Proteus mirabilis*.

### Detection of $\beta$ -lactamase hyperproduction and resistance profile confirmation

The isolates not carrying *mecA* gene although resistant to oxacillin by the disk diffusion test were submitted to the fowling tests to confirm if they were  $\beta$ -lactamase hyperproducers, and to confirm the resistance profile: nitrocefin disk test for  $\beta$ -lactamase hyperproduction; simplex PCR for *mecA* gene detection, cefoxitin by disk diffusion, and amoxicillin/clavulanic acid disk test for resistance confirmation.

### Statistical analysis

The kappa statistic was calculated to assess agreement between the methods used for the identification of *Staphylococcus* sp. A level of significance of 5% was adopted for all tests. Statistical analyses were performed using SSPS software version 19.0 (SSPS Inc., Chicago, IL).

## Results

### Phenotypic identification and susceptibility tests


Identification by the phenotypic method detected 85 (23.0%) *S. aureus* strains and 286 (77.0%) CoNS strains in the 371 blood cultures analyzed. The disk diffusion test revealed oxacillin resistance in 43 (50.6%) *S. aureus* isolates and in 236 (82.5%) CoNS isolates.

### Multiplex PCR

Multiplex PCR was standardized for genotypic identification of the genus *Staphylococcus* (16S rRNA gene), to differentiate coagulase-positive staphylococci and CoNS (*coa* gene), to identify *S. aureus* (*S. aureus*-specific gene), and to detect oxacillin resistance (*mecA* gene) directly from blood culture bottles (Fig. 1).

Amplification was performed on all 371 isolates included in the study. In the case of the 85 *S. aureus* isolates identified phenotypically, there was 100% agreement with the multiplex PCR results, with amplification of the 16S rRNA, *S. aureus* and *coa* genes. Among the 286 CoNS isolates included, 100% agreement between the two methods was only observed in terms of amplification of the 16S rRNA gene.

Amplification of the *mecA* gene was observed in 43 (50.6%) of the 85 *S. aureus* isolates; of these, 42 were resistant to oxacillin by the disk diffusion test and one isolate was susceptible. Among the 42 (49.4%) *mecA* gene-negative isolates, 41 were susceptible by the disk diffusion method and one isolate was resistant. The *mecA* gene was amplified in 225 (78.7%) of the 286 CoNS isolates; of these, 218 were resistant to oxacillin by the disk diffusion test and seven were susceptible. Among the 61 (21.3%) *mecA* gene-negative CoNS isolates, 43 were classified as susceptible by the disk diffusion test and 18 were resistant.

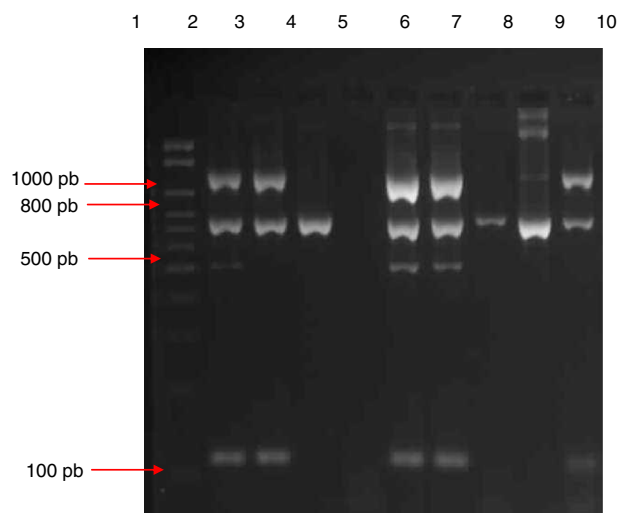

**Fig. 1 – Electrophoresis gel (3% agarose) of the products of multiplex amplification in blood cultures for the detection of *Staphylococcus* spp. and the *mecA* gene. Lane 1: 100–2000 bp Ladder; lane 2: ATCC 33591 (*mecA*-positive *S. aureus*); lane 3: ATCC 25923 (*mecA*-negative *S. aureus*); lane 4: ATCC 12228 (*mecA*-negative *S. epidermidis*); lane 5: negative control; lanes 6 and 7: *mecA*-positive *S. aureus* isolate; lanes 8 and 9: *mecA*-negative CoNS isolate; lane 10: *mecA*-negative *S. aureus* isolate.**

### Detection of $\beta$ -lactamase hyperproduction and resistance profile confirmation

Among the 19 isolates not carrying *mecA* gene although resistant to oxacillin by disk diffusion test, all were positive by nitrocefin disk test and cefoxitin disk diffusion test. On the other hand, six isolates were resistant to amoxicillin/clavulanic acid by disk diffusion test.

### Sensitivity and specificity of the multiplex PCR


In the sensitivity test, amplification of fragments was observed up to a dilution of  $10^{-5}$  ( $10^3$  CFU/mL) for CoNS and of  $10^{-2}$  ( $10^6$  CFU/mL) for *S. aureus*, as shown in Fig. 2. Analysis of specificity using isolates of other species revealed no amplification of any fragments of the genes investigated by multiplex PCR (Fig. 3).

### Costs analysis


The cost of multiplex PCR and the automated Vitek 2 system, the system used for direct bacterial identification in blood cultures at the Laboratory of Microbiology, Department of Internal Medicine, University Hospital, Botucatu Medical School, UNESP, was lower than the phenotypic method (Table 2).

## Discussion

Among the 371 *Staphylococcus* spp. positive blood culture samples included in this study, 23% were positive for *S. aureus*

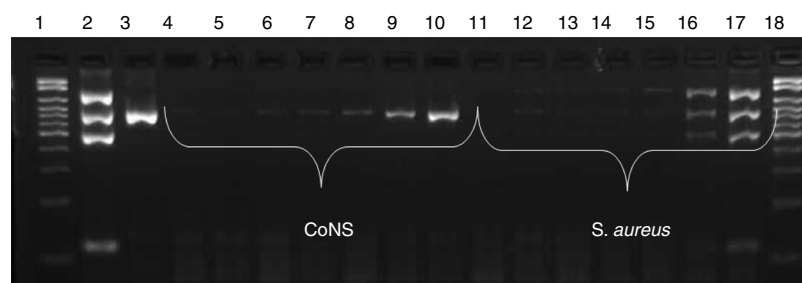

**Fig. 2 – Sensitivity of multiplex PCR.** Electrophoresis gel showing the amplification of different dilutions of CoNS and *S. aureus*. Lane 1: 100–2000 bp molecular weight marker; 2: *mecA*-positive *S. aureus* ATCC; 3: *S. epidermidis* ATCC; 4: CoNS  $10^{-7}$  dilution ( $10^1$  CFU/mL); 5:  $10^{-6}$  ( $10^2$  CFU/mL); 6:  $10^{-5}$  ( $10^3$  CFU/mL); 7:  $10^{-4}$  ( $10^4$  CFU/mL); 8:  $10^{-3}$  ( $10^5$  CFU/mL); 9:  $10^{-2}$  ( $10^6$  CFU/mL); 10:  $10^{-1}$  ( $10^7$  CFU/mL), 11: *S. aureus*  $10^{-7}$  dilution ( $10^1$  CFU/mL); 12:  $10^{-6}$  ( $10^2$  CFU/mL); 13:  $10^{-5}$  ( $10^3$  CFU/mL); 14:  $10^{-4}$  ( $10^4$  CFU/mL); 15:  $10^{-3}$  ( $10^5$  CFU/mL); 16:  $10^{-2}$  ( $10^6$  CFU/mL); 17:  $10^{-1}$  ( $10^7$  CFU/mL); 18: 100–2000 bp molecular weight marker.

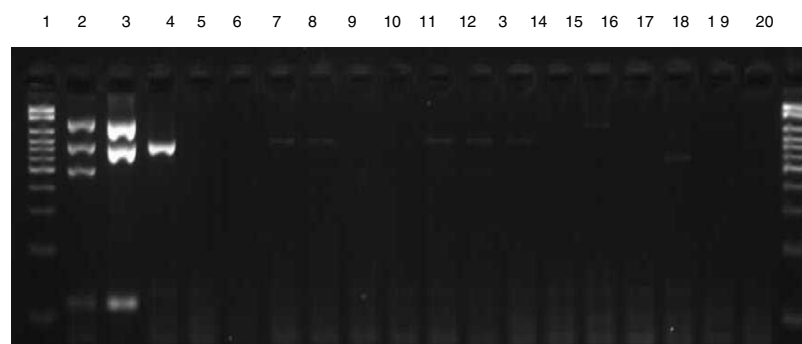

**Fig. 3 – Electrophoresis gel illustrating the specificity of multiplex PCR.** Lane 1: 100–2000 bp Ladder; 2: *mecA*-positive *S. aureus* ATCC; 3: *mecA*-negative *S. aureus* ATCC; 4: CoNS ATCC; 5: *Salmonella* spp.; 6: *Proteus mirabilis*; 7: *Morganella morganii*; 8: *Klebsiella pneumoniae*; 9: *Pseudomonas aeruginosa*; 10: *Acinetobacter baumannii*; 11: *Enterobacter cloacae*; 12: *Enterobacter aerogenes*; 13: *E. coli*; 14: *E. faecalis*; 15: *E. faecium*; 16: *Streptococcus viridans*; 17: *Streptococcus pneumoniae*; 18: *Candida* spp.; 19: Gram-positive bacilli.

**Table 2 – Comparison of the identification costs with the Vitek 2 system and multiplex PCR.**

Method	Cost
Vitek identification	Blood agar: US\$ 0.5
Total: US\$ 6.76 per isolate	MacConkey: US\$ 0.21
	Vitek: US\$ 6.05
Multiplex PCR identification	Extraction: US\$ 2.85
Total: US\$ 4.35 per isolate	Multiplex PCR: US\$ 1.21
	Electrophoresis gel: US\$ 0.29

and 77% were positive for CoNS; of these, 50.6% *S. aureus* isolates and 82.5% CoNS isolates were resistant to oxacillin by the disk diffusion test. In studies conducted with patients from the hospital where the current study was performed,<sup>12</sup> 45.1% *S. aureus* isolates and 72.5% CoNS isolates were resistant to this drug. Other studies also reported high rates of oxacillin-resistant *Staphylococcus* spp. isolates.<sup>13,14</sup> In view of this increase in resistant isolates, treatment options have narrowed down to glycopeptides and new synthetic drugs such

as linezolid.<sup>15</sup> In addition to being expensive and toxic, these drugs select resistant strains. In some countries there are reports of *Staphylococcus* spp. resistant to vancomycin, which increasingly limits the therapeutic options.<sup>16,17</sup>

In view of these considerations, the faster the results of culture and antimicrobial susceptibility testing are released, the faster the physician can adjust treatment, reducing the risks and harm caused by the organism to the patient. In the present study, a multiplex PCR assay that permitted direct detection of oxacillin-resistant *S. aureus* (MRSA) in blood cultures was developed using an extraction technique that was effective and able to eliminate interfering elements present in blood. Bloodstream infections caused by MRSA complicate the prognosis of the patient, increasing the length-of-hospital stay, mortality rate, number of invasive procedures, and hospitalization costs.<sup>18</sup>

Investigation of the *coa* gene included in the multiplex assay for detection of all coagulase-positive staphylococci and the use of the *S. aureus*-specific SAU primer permit to establish whether the isolate is *S. aureus* or not.

In addition to the detection of *Staphylococcus* spp., the multiplex assay proposed in this study also included investigation of the *mecA* gene to detect oxacillin resistance, in order to guide patient treatment at the time of identification. Pereira et al.<sup>19</sup> developed a multiplex PCR assay that directly identified three *Staphylococcus* spp. species, *S. aureus*, *S. epidermidis* and *S. haemolyticus*, and the *mecA* gene in blood cultures, but this identification was restricted to these species. The multiplex assay standardized in this study permits the detection of all staphylococcal species isolated from bacteremias. The multiplex PCR was tested using 371 samples, 13 blood culture samples containing other bacterial species and bacterial DNA of other species directly from bacterial culture, showed good sensitivity and specificity.

In addition to being specific, our multiplex PCR assay exhibited a detection threshold of MRSA of 10<sup>6</sup> CFU/mL. Similar thresholds have been reported in other studies.<sup>20</sup> The threshold may decrease with increasing number of amplified genes, but even so the threshold found in this study was within the proposed range of detection since, according to Pereira et al.,<sup>20</sup> positive blood cultures present a growth of about 10<sup>9</sup> CFU/mL. The only discrepancy observed in this study was the detection of the *mecA* gene by the standardized multiplex PCR assay and susceptibility to oxacillin in the phenotypic test, with the *mecA* gene not being detected in 19 isolates resistant to oxacillin (one *S. aureus* isolate and 18 CoNS isolates). In these isolates, the *mecA* gene was detected by simplex PCR, confirming the results of multiplex PCR. This discrepancy has also been reported in other studies<sup>20-23</sup> and may be related to other types of resistance such as  $\beta$ -lactamase hyperproduction or modification of another PBP. Furthermore, eight isolates were positive for the *mecA* gene and were susceptible in the phenotypic test (one *S. aureus* isolate and 7 CoNS isolates). These findings highlight the importance of genotypic techniques for the detection of oxacillin resistance, but do not rule out the need for other phenotypic techniques to initiate more specific and effective treatment.

The implementation of a molecular biology technique such as multiplex PCR to assist in the rapid diagnosis of bloodstream infections may be associated with high costs for the institution. A cost analysis performed in the present study showed that the identification of species in culture, i.e., after detection of a positive blood culture with the Bactec system, its seeding on culture plates and identification, which is done with the Vitek 2 system at the Laboratory of Microbiology in Botucatu Medical School has an average cost of US\$ 6.76. In the case of multiplex PCR, which does not require seeding of the blood culture for isolation of the microorganisms since it uses direct identification from blood culture bottles, DNA extraction and PCR amplification for detecting *Staphylococcus* spp., *S. aureus*, and the *mecA* gene were estimated to cost US\$ 4.35 per isolate.

The multiplex PCR assay developed here was found to be sensitive, specific, rapid and less expensive than the phenotypic technique used, and showed good agreement with the phenotypic results. This method could be used in clinical laboratories for rapid identification and initiation of specific and effective treatment, reducing patient mortality and morbidity. Furthermore, this method may reduce the misuse of other antimicrobial classes that are more expensive and toxic, thus

contributing to the selection of antibiotic-resistant *Staphylococcus* spp.

## Conflicts of interest

The authors declare no conflicts of interest.

## Acknowledgements

São Paulo Research Foundation (FAPESP Grant 2010/14250-0) and National Council for Scientific and Technological Development (CNPq) for financial support.

## REFERENCES

1. Russel JA. Management of sepsis. *N Engl J Med.* 2006;355:1699-713.
2. Magill SS, Edwards JR, Bamberg W, et al. Multistate point-prevalence survey of health care-associated infections. *N Engl J Med.* 2014;370:1198-208.
3. Euzebey J. List of Prokaryotic Names with Standing in Nomenclature: LPSN; 2017. Available from: <http://www.bacterio.net/s/staphylococcus.html>
4. Bannerman TL. *Staphylococcus, Micrococcus and the other catalase-positive cocci that grow aerobically.* In: Murray PR, Baron EJ, Jorgensen JH, Pfaller MA, Tenover FC, Tenover FC, editors. *Manual of clinical microbiology.* 8th ed. Washington, DC: ASM Press; 2003.
5. Springer B, Orendi U, Much P, et al. Methicillin-resistant *Staphylococcus aureus*: a new zoonotic agent? *Wien Klin Wochenschr.* 2009;121:86-90.
6. Hackbarth CJ, Chambers HF. Methicillin-resistant *Staphylococci*: genetics and mechanisms of resistance. *Antimicrob Agents Chemother.* 1989;33:991-4.
7. Lim TT, Coombs GW, Grubb WB. Genetic organization of *mecA* and *mecA*-regulatory genes in epidemic methicillin-resistance *S. aureus* from Australia and England. *J Antimicrob Chemother.* 2002;50:819-24.
8. Kaiser TD, Pacheco FC, Lima AA, Pereira EM, Santos KR, Nunes APF. Avaliação de métodos comumente usados em laboratório para a determinação da suscetibilidade à oxacilina entre amostras de *Staphylococcus* spp., isoladas de um Hospital de Vitória, estado do Espírito Santo. *Soc Bras Med Trop.* 2010;43:298-303.
9. Hogg GM, McKenna JP, Ong G. Rapid detection of methicillin-susceptible and methicillin-resistant *Staphylococcus aureus* directly from positive BacT/Alert® blood culture bottles using real-time polymerase chain reaction: evaluation and comparison of 4 DNA extraction methods. *Diagn Microbiol Infect Dis.* 2008;61:446-52.
10. Fredricks DN, Relman DA. Improved amplification of microbial DNA from blood cultures by removal of the PCR inhibitor sodium polyacrylate. *J Clin Microbiol.* 1998;36:2810-6.
11. Clinical and Laboratory Standards Institute (CLSI). Approved standards: M100-S22 Performance standards for antimicrobial susceptibility testing. Wayne, PA: CLSI; 2012.
12. Martins A, Pereira VC, Cunha MLRS. Oxacillin resistance of *Staphylococcus aureus* isolated from the university hospital of Botucatu Medical School in Brazil. *Chemotherapy.* 2010;56:112-9.
13. Cuevas O, Cercenado E, Goyanes MJ, et al. *Staphylococcus* spp. in Spain: present situation and evolution of antimicrobial

- resistance (1986–2006). *Enferm Infecc Microbiol Clin*. 2008;26:269–77.
14. Cunha MLRS, Lopes CAM. Estudo da produção de beta-lactamases e sensibilidade às drogas em linhagens de *Stafilococos* coagulase-negativos isolados de recém-nascidos. *J Bras Patol Med Lab*. 2002;38:281–90.
  15. Woods W, Ramotar K, Lem P, Toye B. Oxacillin susceptibility testing of coagulase-negative staphylococci using the disk diffusion method and the Vitek GPS card. *Diagn Microbiol Infect Dis*. 2002;42:291–4.
  16. Chang S, Sievert DM, Hageman JC, et al. Infection with vancomycin-resistant *Staphylococcus aureus* containing the vanA resistance gene. *N Engl J Med*. 2003;348:1342–1347.
  17. Cunha MLRS. *Staphylococcus aureus* and coagulase-negative staphylococci: virulence antimicrobial resistance and molecular epidemiology. New York: Nova Science Publishers; 2014.
  18. McHugh CG, Riley LW. Risk factors and costs associated with methicillin-resistant *Staphylococcus aureus* bloodstream infections. *Infect Control Hosp Epidemiol*. 2004;25:425–30.
  19. Pereira EM, Schuenck RP, Malvar KL, et al. *Staphylococcus aureus*, *Staphylococcus epidermidis* and *Staphylococcus haemolyticus*: methicillin-resistant isolates are detected directly in blood cultures by multiplex PCR. *Microbiol Res*. 2010;165:243–9.
  20. Pereira VC, Martins A, Rugolo LMSS, Cunha MLRS. Detection of oxacillin resistance in *Staphylococcus aureus* isolated from the neonatal and pediatric units of a Brazilian teaching hospital. *Clin Med Pediatr*. 2009;3:23–31.
  21. Schimitz FJ, Mackenzie CR, Hofman B, et al. Specific information concerning taxonomy, pathogenicity and methicillin resistance of staphylococci obtained by multiplex PCR. *J Med Microbiol*. 1997;46:773–8.
  22. Caierão J, Superti S, Dias CA, d'Azevedo PA. Automated systems in the identification and determination of methicillin resistance among coagulase negative Staphylococci. *Mem Inst Oswaldo Cruz*. 2006;101:277–80.
  23. Kilic A, Muldrew KL, Tang YW, Baustaoglu AC. Triplex real-time polymerase chain reaction assay for simultaneous detection of *Staphylococcus aureus* and coagulase-negative staphylococci and determination of methicillin resistance directly from positive blood culture bottles. *Diagn Microbiol Infect Dis*. 2010;66:349–55.
  24. Riffon R, Sayasith K, Khalil H, Dubreuil P, Drolet M, Lagacé J. Development of a rapid and sensitive test for identification of major pathogens in bovine mastitis by PCR. *J Clin Microbiol*. 2001;39:2584–9.
  25. Mason WJ, Blevins JS, Beenken K, Wibowo N, Ojha N, Smeltzer MS. Multiplex PCR protocol for the diagnosis of staphylococcal infection. *J Clin Microbiol*. 2001;39:3332.
  26. Kearns AM, Siders PR, Wheeler J, Freeman R, Steward M. Rapid detection of methicillin-resistant *Staphylococci* by multiplex PCR. *J Hosp Infect*. 1999;53:33–7.
  27. Murakami K, Minamide W, Wada K, Nakamura E, Teraoka H, Watanabe S. Identification of methicillin-resistant strains of *Staphylococci* by polymerase chain reaction. *J Clin Microbiol*. 1991;29:2240–4.